


**TCTAP A-083****Incomplete Stent Apposition Causes High Shear Flow Disturbances and Delay in Neointimal Coverage as a Function of Strut to Wall Detachment Distance: Implications for Stent Optimization**

Nicolas Foin,<sup>1</sup> Juan Luis Gutierrez Chico,<sup>2</sup> Shimpei Nakatani,<sup>3</sup> Ryo Torii,<sup>4</sup> Renick Lee,<sup>5</sup> Sayan Sen,<sup>1</sup> Ricardo Petraco,<sup>1</sup> Philip Wong,<sup>5</sup> Carlo Di Mario,<sup>6</sup> Yoshinobu Onuma,<sup>7</sup> Justin E. Davies,<sup>1</sup> Patrick W. Serruys<sup>8</sup>

<sup>1</sup>Imperial College London, United Kingdom; <sup>2</sup>Charite Hospital, Germany; <sup>3</sup>Sakurabashi Watanabe Hospital, Japan; <sup>4</sup>University College London, United Kingdom; <sup>5</sup>National Heart Centre, Singapore; <sup>6</sup>Royal Brompton Hospital, United Kingdom; <sup>7</sup>Thorax Center, Netherlands; <sup>8</sup>Imperial College London, Netherlands

**BACKGROUND** Lack of re-endothelialization and neointimal coverage on stent struts has been put forward as the main underlying mechanism leading to late stent thrombosis. Incomplete Stent Apposition (ISA) has been frequently observed in patients with very late stent thrombosis after DES implantation, suggesting a role of ISA in the pathogenesis of this adverse event. The aim of this study was to evaluate the impact of different degrees of ISA severity on abnormal shear rate and healing response with coverage, due to its potential implications for stent optimization in clinical practice. We characterized flow profile and shear distribution in different cases of ISA with increasing strut-wall detachment distance (ranging from 100  $\mu$ m to 500  $\mu$ m). In-vivo impact on strut coverage was assessed retrospectively using Optical Coherence Tomography evaluation on 72 stents (48 patients) sequentially at baseline and after 6 months follow-up.

**RESULTS** Protruding strut and strut malapposed with moderate detachment (ISA detachment distance < 100  $\mu$ m) have minimal disturbance to blood flow as compared with floating strut that has more significant ISA distance. Analysis of coverage revealed an important impact of baseline strut-wall ISA distance on the risk of incomplete strut coverage at follow-up. Malapposed segments with an ISA detachment < 100  $\mu$ m at baseline showed complete strut coverage at follow-up whereas segments with a maximal ISA detachment distance of 100-300  $\mu$ m and >300  $\mu$ m had 6.1 % and 15.7 % of their struts still uncovered at follow-up respectively ( $p < 0.001$ ). Finally, a study performed in-vivo animal model, in which a series of stent were implanted with a controlled under-expansion, confirmed the impact of stent apposition as well as platform design on the coverage process.

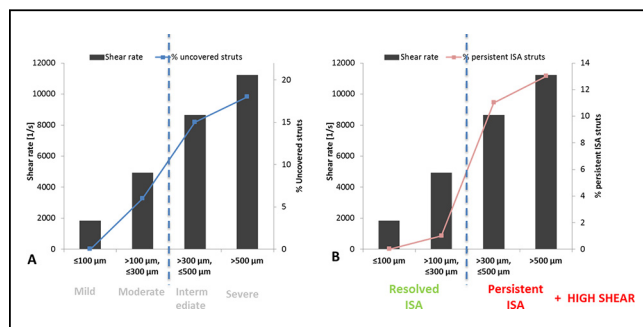

**CONCLUSION** Flow disturbances and risk of delayed strut coverage both increase with ISA detachment distance. Insights from this study are important for understanding malapposition as a quantitative, rather than binary phenomenon (present or absent), and to define the threshold of ISA detachment that might benefit from optimization during stent implantation.

### NON-INVASIVE CARDIAC IMAGING: CTA, MRI, 3D-ECHO, AND OTHER (TCTAP A-084 TO TCTAP A-085)


**TCTAP A-084****Lesion-Specific Myocardial Mass: A New Index for Diagnosis and Treatment of Coronary Artery Disease**

Hyung Yoon Kim,<sup>1</sup> Jin-Ho Choi<sup>1</sup>


<sup>1</sup>Samsung Medical Center, Korea (Republic of)

**BACKGROUND** Accurate quantification of the myocardial mass by coronary computed tomography angiography (CCTA) has become

available. And lesion-specific myocardial mass (LMM) could be estimated with clinical applications of allometric scaling law. The aim of this study was to estimate the influence of the amount of lesion-specific myocardial mass on the diagnostic performance of %DS to predict functional ischemia defined as fractional flow reserve (FFR)  $\leq 0.80$ .

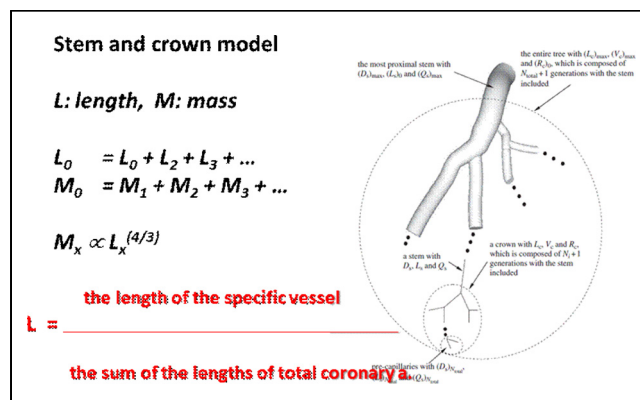

**METHODS** CCTA and FFR were performed to evaluate 208 lesions in 132 patients. Index of myocardial ischemia was defined as FFR  $\leq 0.80$ . Total and lesion-specific myocardial mass was estimated using CCTA measurements based on allometric scaling method. And the lesion-specific myocardial mass was defined as each myocardial mass per each supply vessel. Bivariate analysis was performed to estimate correlation between FFR and %DS in accordance with the amount of lesion-specific myocardial mass.

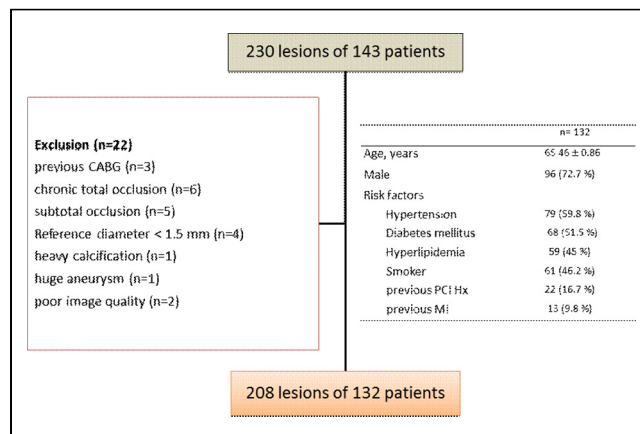

**RESULTS** Ischemia was observed in 102 lesions. The mean FFR value was  $0.75 \pm 0.11$ . Lesions with FFR  $\leq 0.8$  had less minimal luminal diameter and more % DS of ICA.

And also had less MLA and more %DS of CCTA. Mean total myocardial mass of CCTA was 108.20 (g) and mean lesion-specific myocardial mass was 36.51 (g). We found that, at the same anatomic severity of stenosis, larger LMM tend to produce more functionally significant ischemia. Lesions with larger LMM and/or smaller MLD produced more significant functional ischemia. Further analysis using LMM divided by MLD as a new index was performed to assess its diagnostic performance to predict functionally significant ischemia. With the best cut-off value of 38.4, the AUC of the ROC were 0.79 with 59% of sensitivity and 87% of specificity.